

# **CERTIFICATE OF ANALYSIS**

Agilent Product Name: Oligonucleotide Resolution Standard

Agilent Part No: 5190-9028 Lot or Batch No: 233628911 Expiration Date: 11-JAN-2019

#### Instructions


It is recommended to reconstitute the standard with 1000 µl of water

#### **Product Specifications/Analysis**

All individual oligonucleotides are purified by HPLC. Molecular weight is determined for each individual oligonucleotide using ESI mass spectrometry. Amount is determined by HPLC analysis of the mixture using an independently prepared calibration curve.

| Sequence<br>Name | Sequence                                   | Purity<br>Guarantee | Molecular<br>Weight (Da) | Amount (nmole) |
|------------------|--|---------------------|--------------------------|----------------|
| 14mer            | rCrArCrUrGrArArUrArCrCrArArU               | 85% <u>&gt;</u>     | 4398.4                   | 2              |
| 17mer            | rUrCrArCrArCrUrGrArArUrArCrCrArArU         | 85% <u>&gt;</u>     | 5338.3                   | 2              |
| 20mer            | rUrCrArUrCrArCrArCrUrGrArArUrArCrCrArArU   | 85% <u>&gt;</u>     | 6279.1                   | 2              |
| 21mer            | rGrUrCrArUrCrArCrArCrUrGrArArUrArCrCrArArU | 85% <u>&gt;</u>     | 6624.7                   | 4              |

#### Chromatogram

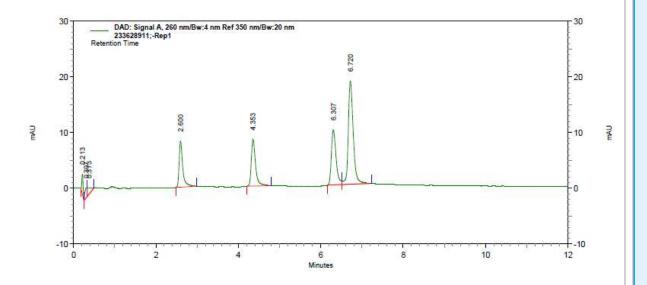

# **CERTIFICATE OF ANALYSIS**

### **Testing Conditions:**

Column: Agilent AdvanceBio Oligonucleotides Column, 2.1 x 50mm Mobile Phase A: 100mM TEAA in water

Mobile Phase B: 100mM TEAA in acetonitrile

Gradient: 6 to 8% B in 12 minutes

Stop Time: 13 minutes Flow: 0.6 mL/min

Column Temperature: 65 °C Injection Volume: 0.5 µL Detection: UV @ 260 nm

### **Manufacturing Statement**

These oligonucleotides were manufactured and verified under a quality system registered to ISO 9001:2008.

Date of Manufacture: 11-JAN-2018